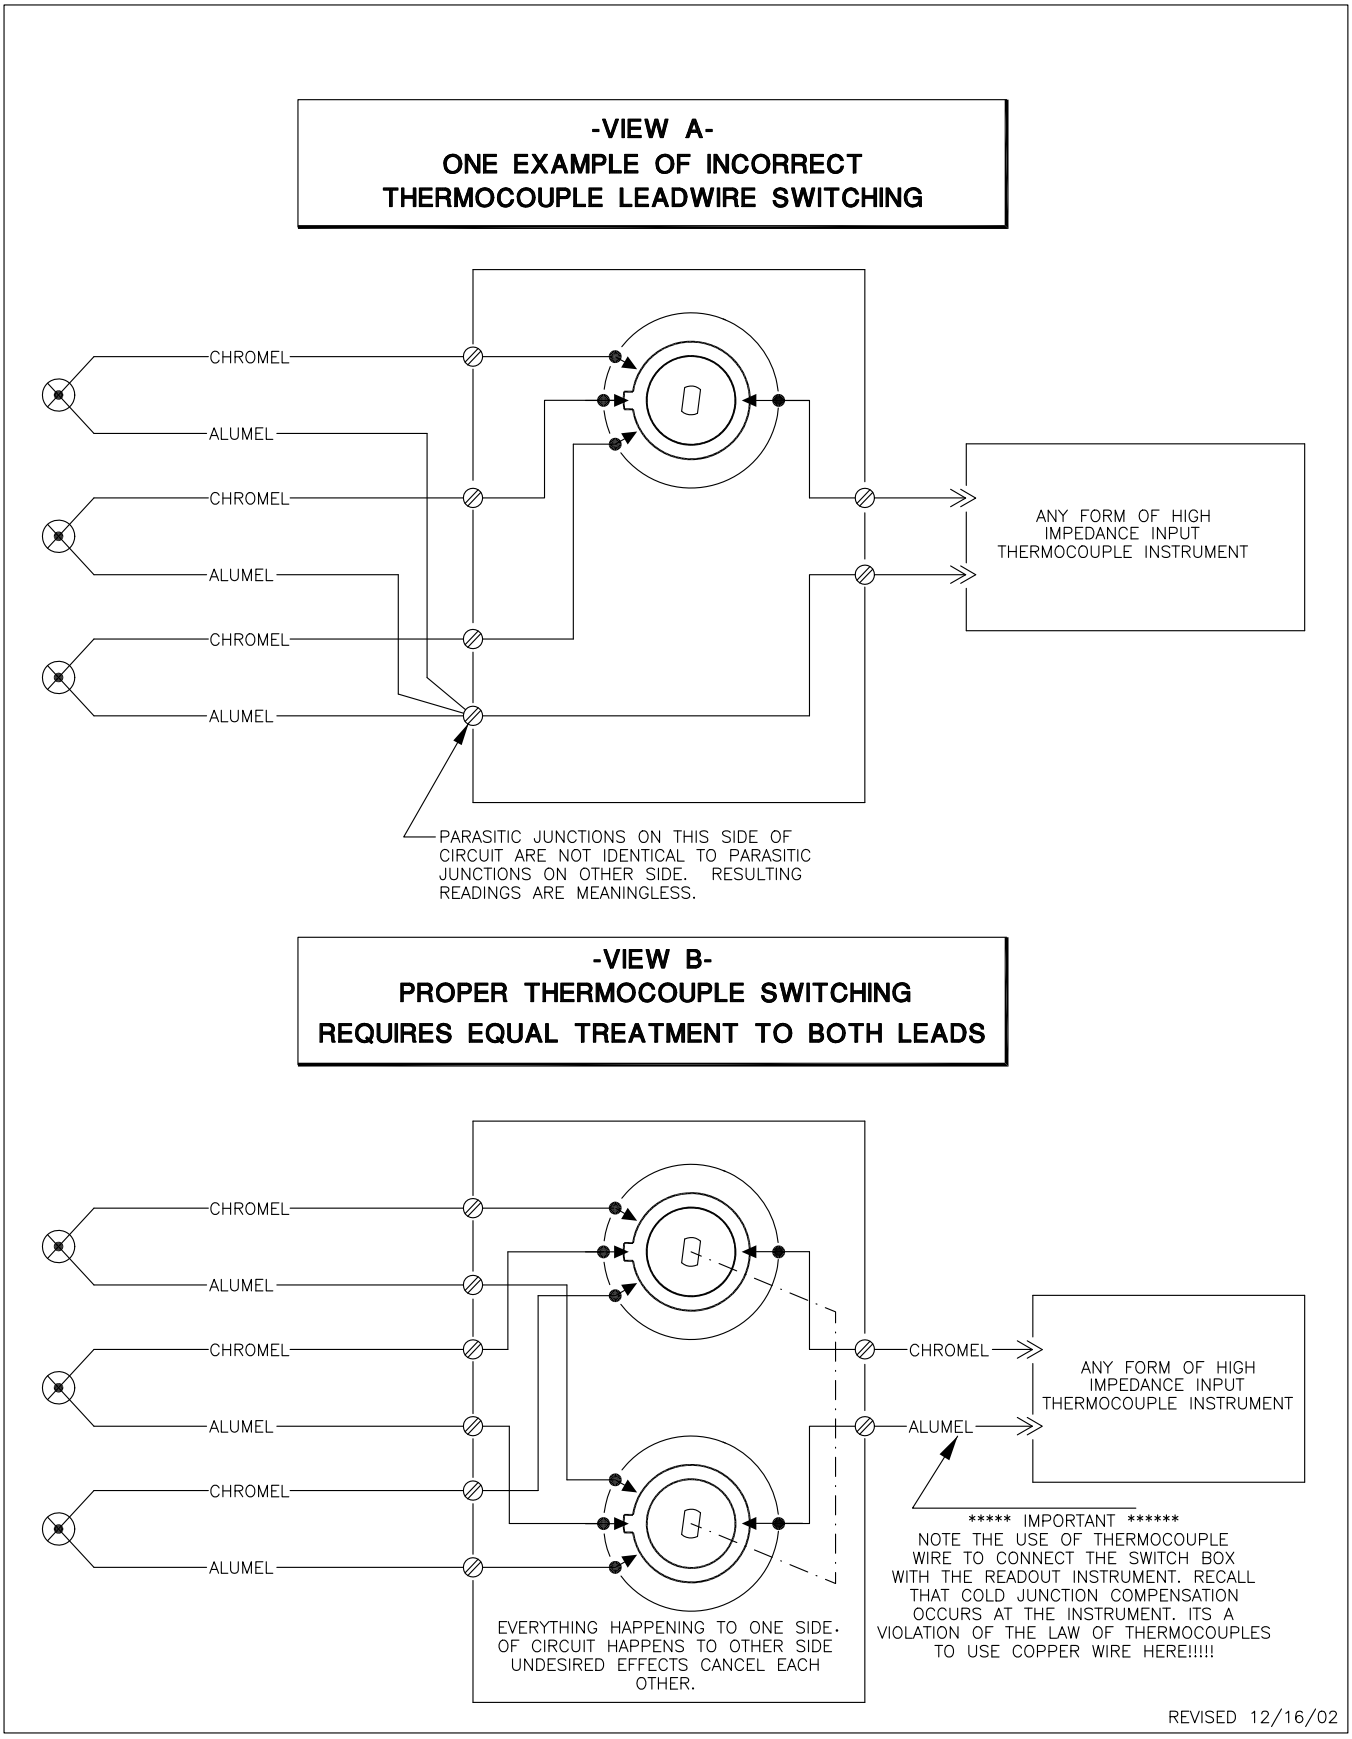

Figure 14-11. Switching Multiple Thermocouples to a Single Instrument.